

## **EN** Installation instructions Shower trolley 346



### **EN** Products


#### **Shower and Changing Tables**

Height Adjustable Shower Trolley Granberg 346

1. Mechanical construction
2. Delivery modules
3. Electrical connection
4. Location of the shower trolley
5. Functional test

## 1. Mechanical construction

1. Motor
2. Mattress
3. Foldable gates
4. Lockable wheels

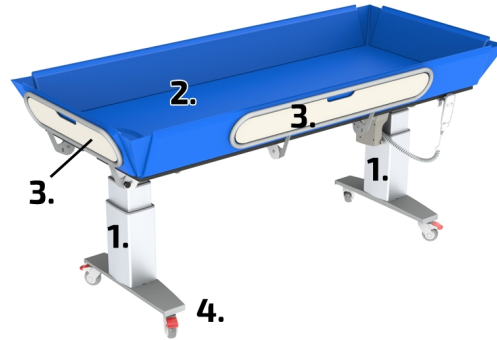

## 2. Delivery modules

The shower trolley is delivered assembled on a pallet.

## 3. Electrical connection

The shower trolley must be connected to a nearby main switch.

If the table is installed in a wet room, wet room regulations must be observed. The motor power supply must always be provided with an earth fault circuit breaker.

Connect the table to a 230V 50Hz power outlet. The outlet must be out of reach of children, remembering that the shower trolley surface can be raised and lowered.

Cables must be routed and fixed with care to avoid the risk of pinching.

\* Power requirement 230 W.

**Electrical connections must be made by a qualified electrician.**

## 4. Location of the shower trolley

The shower trolley may only be placed in a space equipped with a floor drain.

Take care to locate the shower trolley so as to avoid pinching hazards. The distance to any adjacent fitting must be at least 50 mm. If the distance from the shower trolley to a wall or an adjacent fitting is less than 50 mm, a pinching hazard exists.

It is the responsibility of the installer and the user to locate the shower trolley so that pinching hazards are avoided.

## 5. Functional test

- Minimum distance to any adjacent fitting must be at least 50 mm.  
If the distance from the changing surface to a wall or an adjacent fitting is less than 50 mm, a pinching hazard exists.
- Run the shower trolley down and up all the way to respectively end position. Check that it moves freely, without hindrance and jarring sounds.
- Check that no cables are jammed.
- **Shower trolley with two motors has to be synchronized:**  
Press the down button for 5 seconds until the control box clicks. When the control box clicks the synchronisation is ok.